


Central Service Unit

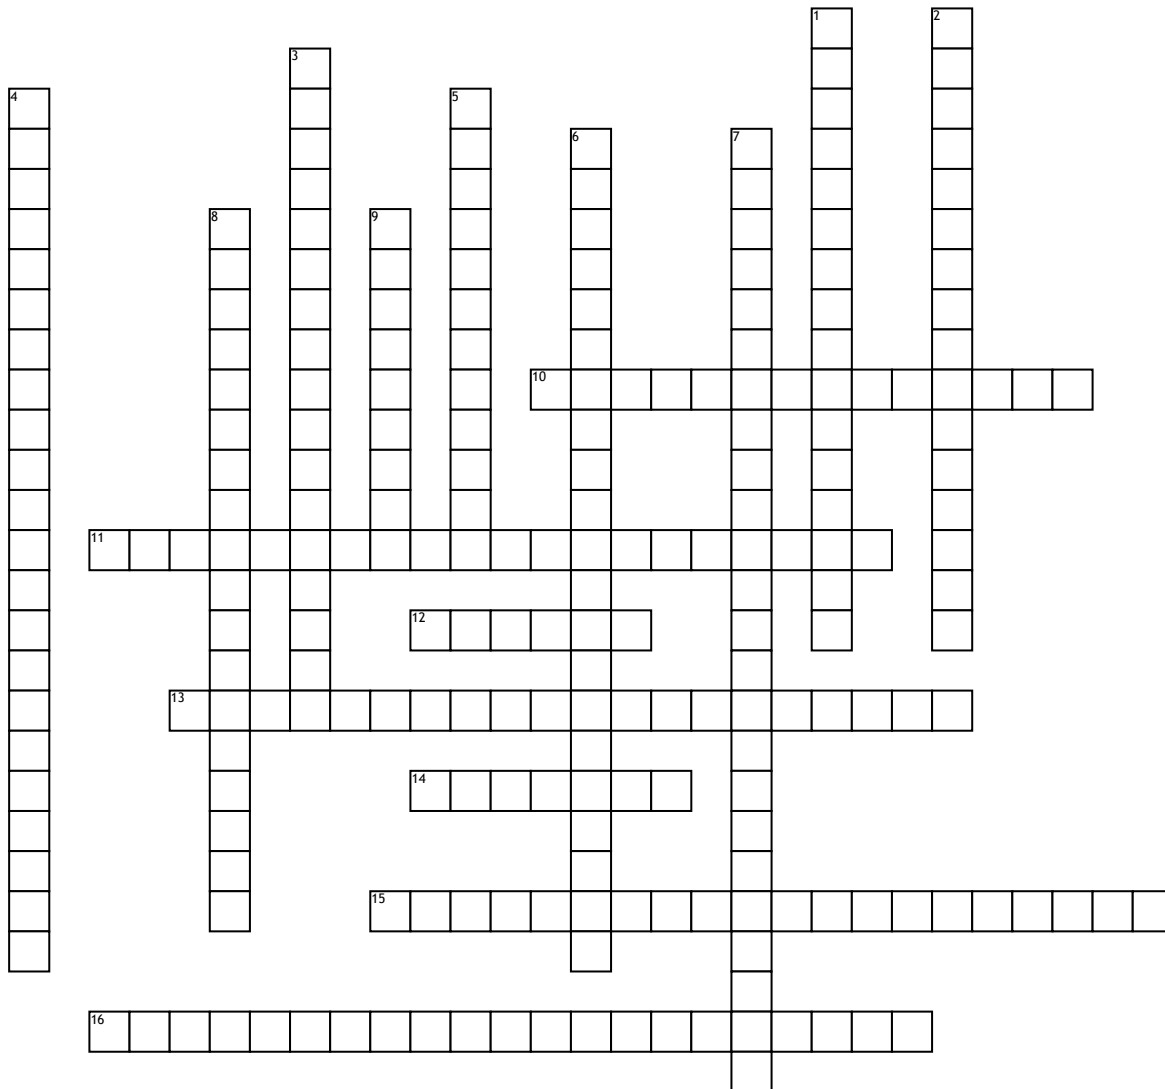

Across

10. Containing maximum amount of h2o vapor when sterilizing
 11. Container that hold and protect instrument sets for steriliation
 12. Plain weave cotton fabirc for packaging
 13. use by date.
 14. Evidence of moisture after sterilaztion
 15. Prerapring a medical device immediately before patient care use

16. Sterile unit damage

Down

1. Dry and hoter than saturated steam for sterilization.
 2. Absorbment material allowing air and steam removal
 3. The monitoring device for proof of sterilization
 4. An agent used to simulate predetermined spore conditions
 5. Where inspection and packagaing are preformed?

6. Designed for urgent situations when sterilizing and storing

7. Sterilization process done quickly for patient care items
 8. Last step when sealing a container ready for sterilaztion step.
 9. Contaminated objects due to microrganisms