


Name: _____

Date: _____

Impella Ventricular Assist Device

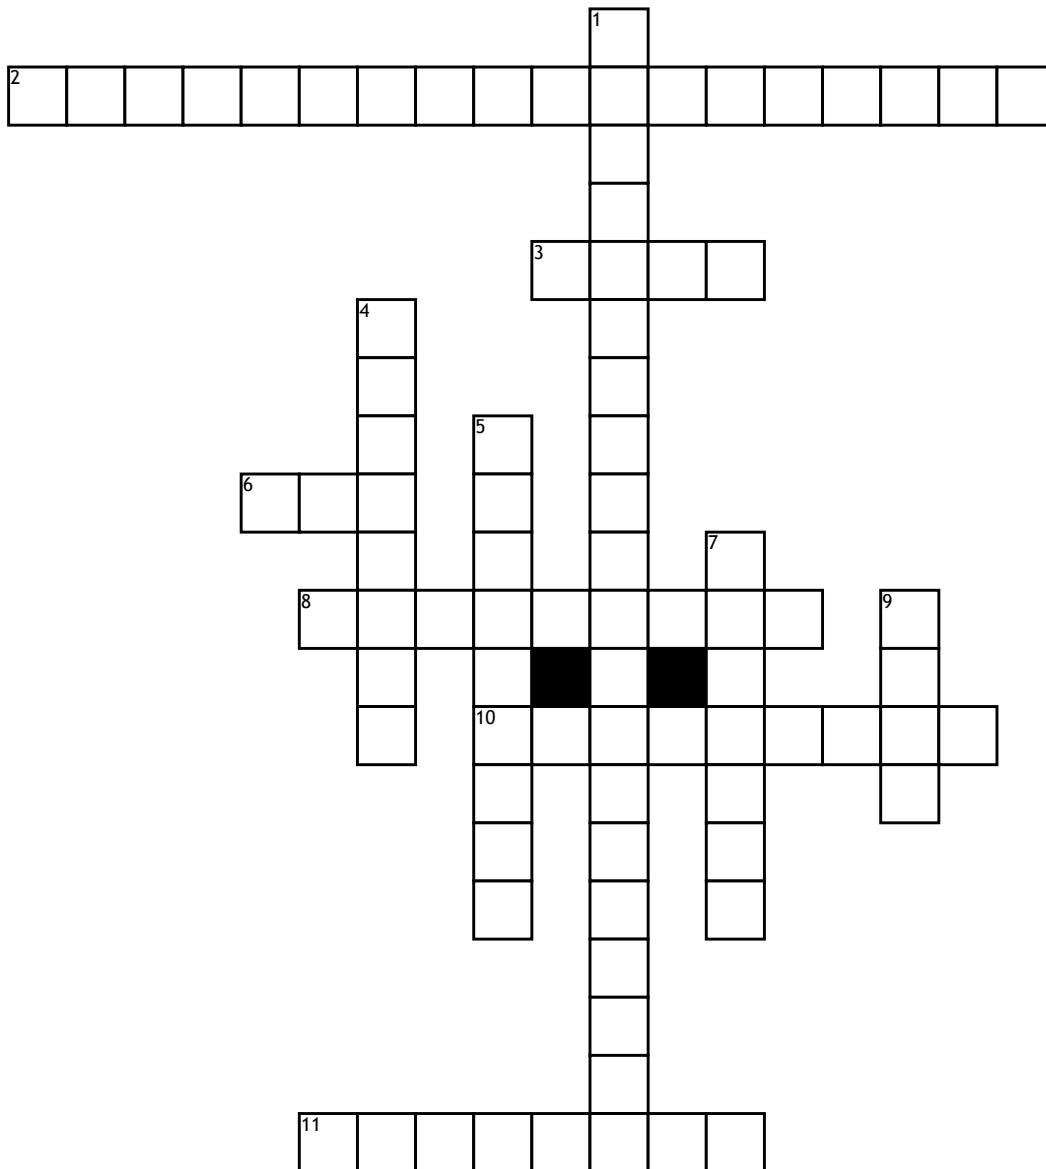

Across

2. Best indicator of mortality for patients in cardiogenic shock
 3. Pulmonary Artery Pulsatility Index - reflects RV function
 6. Therapeutic level is 160-180 seconds
 8. Impella _____ oxygen demand of the myocardium
 10. One type of stiff wire used for Impella placement

11. _____ fr sheath is used for Impella placement

Down

1. Target is 60-65mmHg
 4. AO waveform does this after Impella therapy started
 5. Impella _____ cardiac output and end organ perfusion
 7. Standard configuration uses D5W with 25,000 units _____
 9. Impella allows the LV to _____