

Name: \_\_\_\_\_

Date: \_\_\_\_\_

# Infection Control

## Across

2. you should never touch the dialysis machine with your \_\_\_\_\_


5. \_\_\_\_\_ are not reusable, and cannot be hanging in the POD for multiple uses.

6. All disposable supplies brought into the patient's "room" are \_\_\_\_\_ when the patient is discharged from the POD

8. \_\_\_\_\_ are required when touching the patients curtains

9. the treatment area is \_\_\_\_\_ disinfected while the patient is in the POD

10. Heparin vials expire \_\_\_\_\_ days after opening?

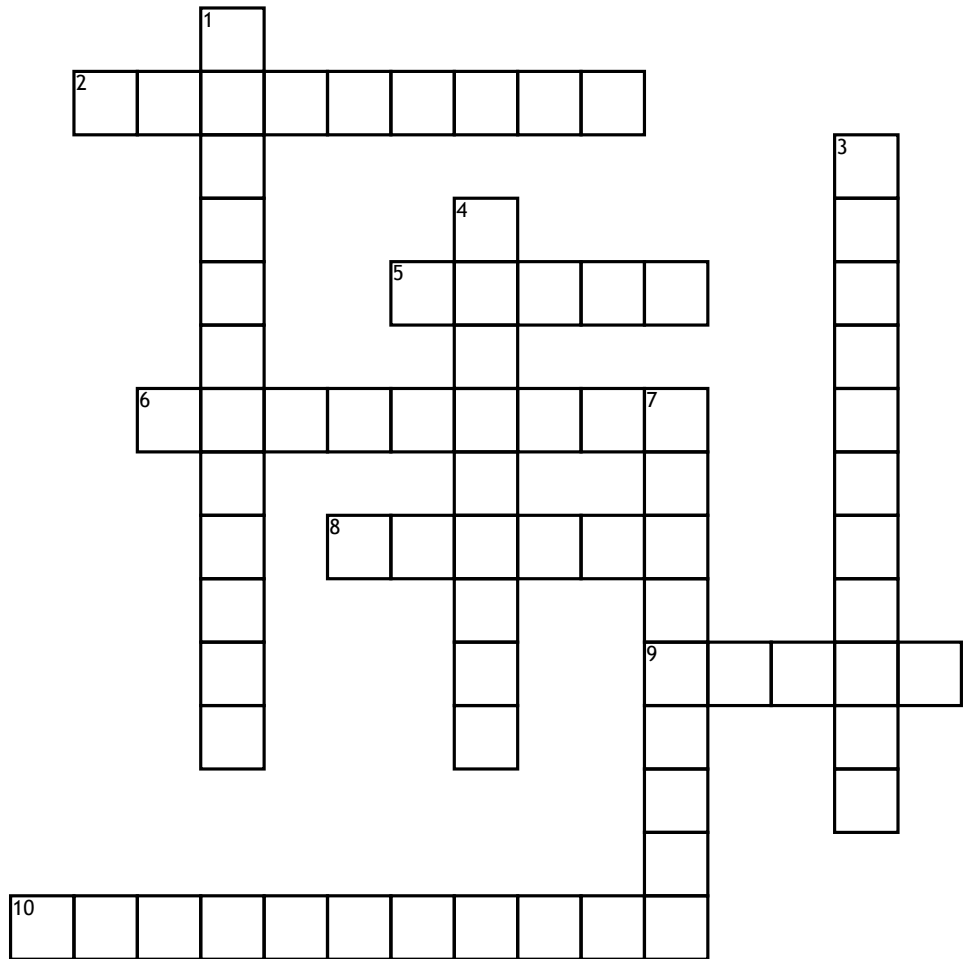

## Down

1. Infection control precautions are designed to prevent \_\_\_\_\_ of bloodborne viruses and pathogens among patients.

3. the \_\_\_\_\_ is disinfected before the machine is

4. dialysis machines may not recirculate for more than \_\_\_\_\_

7. \_\_\_\_\_ hands before applying and after removing gloves

