


# Laser Safety

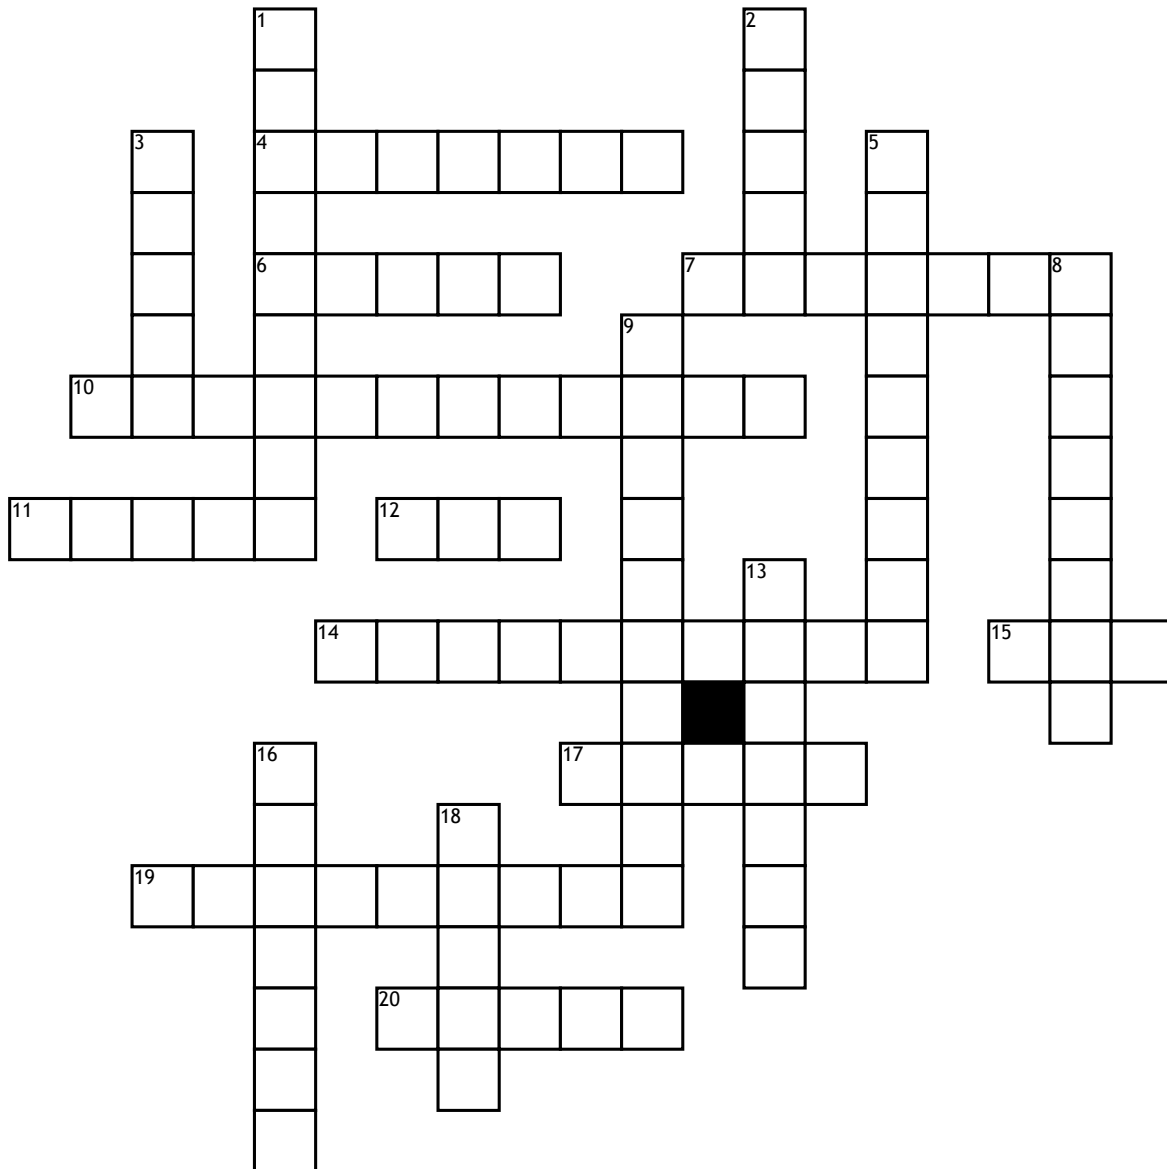

**Across**

- 4. \_\_\_\_\_ lenses do not provide sufficient eye protection in laser cases
- 6. Employees should wear a laser mask in cases that generate surgical \_\_\_\_\_
- 7. During laryngotracheal laser surgery, a 60ml \_\_\_\_\_ of water or NaCl should be available on the mayo stand
- 10. A laser safe \_\_\_\_\_ tube should be used when oral, nasopharyngeal or laryngotracheal laser procedures are being performed
- 11. Laser eyewear should be hung on the outside \_\_\_\_\_ for staff entering a room where a laser is in use
- 12. When the laser is left unattended for a substantial period of time, the laser shall be turned off and \_\_\_\_\_ removed

- 14. When performing laser surgery, the patient's eyes must be \_\_\_\_\_ with a water base artificial tear solution, or taped closed, and covered with moist eye pads
- 15. \_\_\_\_\_ towels should be used for draping around the surgical site
- 17. \_\_\_\_\_ must be posted on all doors of area where laser is in use
- 19. \_\_\_\_\_ preps should be avoided in laser cases.
- 20. the operating surgeon should have the laser foot \_\_\_\_\_ only and none others to operate

**Down**

- 1. Using \_\_\_\_\_ during carbon dioxide laser surgery prevents the beam from striking unintended tissue
- 2. Laser Safety Crossword Puzzles make me \_\_\_\_\_

- 3. A \_\_\_\_\_ fire extinguisher must be available in the surgical suite during a laser case
- 5. Sponges used on the surgical field must be \_\_\_\_\_.
- 8. Instruments used in the immediate vicinity of the laser should be \_\_\_\_\_
- 9. All \_\_\_\_\_ surfaces in the room should be covered prior to laser use.
- 13. The laser should be in \_\_\_\_\_ position at all times when not being used by the surgeon
- 16. All employees must wear laser \_\_\_\_\_ to prevent injury to the eyes.
- 18. A basin of \_\_\_\_\_ should be on the sterile field during all laser cases