


Name: \_\_\_\_\_ Date: \_\_\_\_\_

# Sterile Processing Service

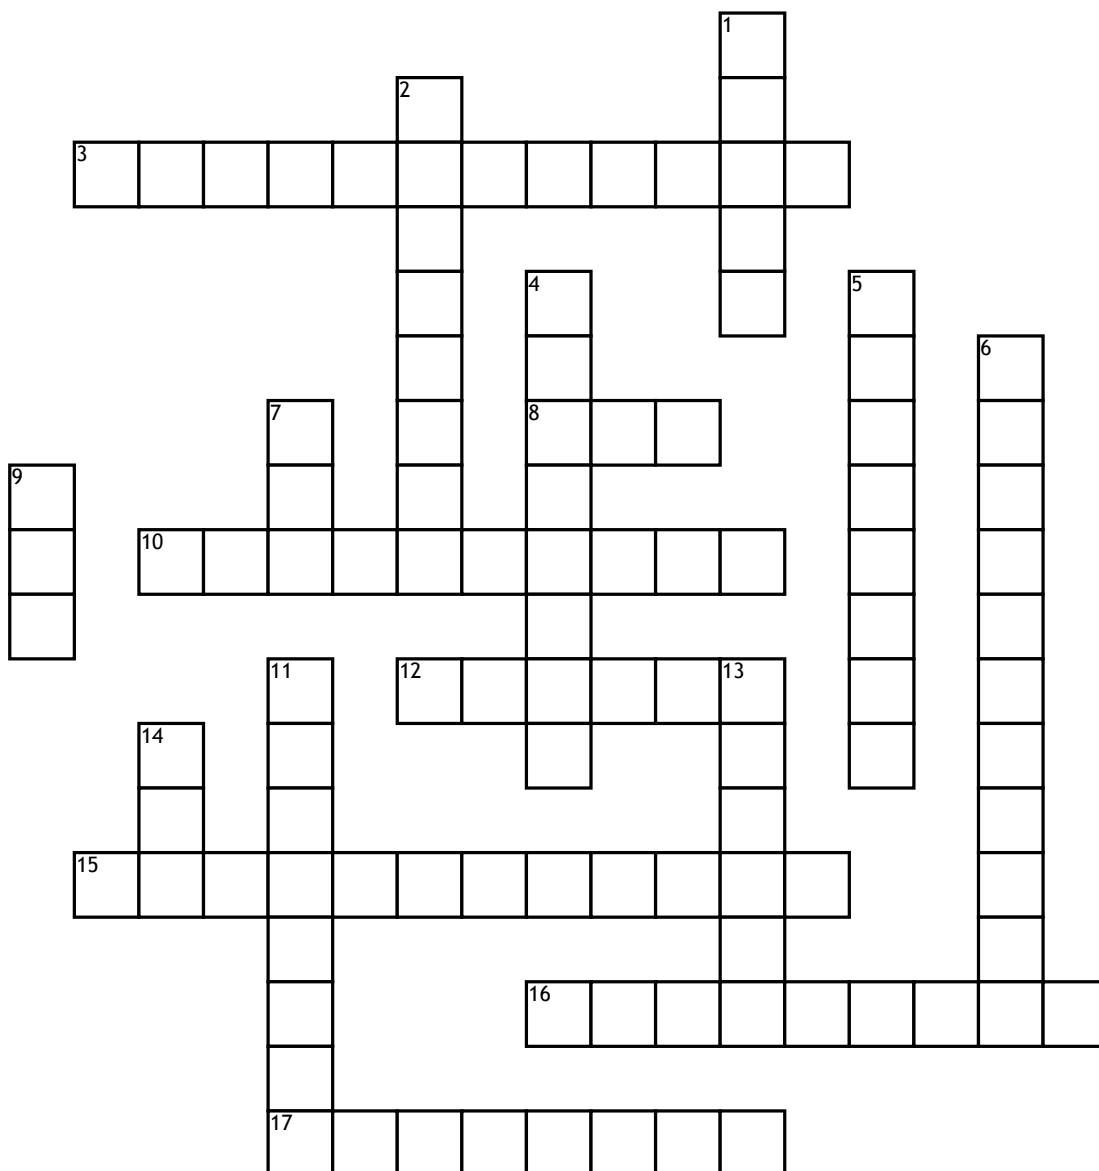

## Across

3. RME is considered sterile unless an event occurs deeming it compromised

8. Any medical equipment to be reused from one patient to another

10. Clean to Dirty

12. Must be 12 mil thick

15. Spaulding Classification that is defined as coming into contact with mucous membranes or non-intact skin

16. Occurs regularly to ensure everyone knows what to do in case of a fire

17. Wrapping technique frequently used for smaller trays

## Down

1. Type of sterilizer used for items that are not heat sensitive

2. Spaulding Classification that is defined as Introduced into the sterile body or blood stream

4. Dirty to Clean

5. Pressure of Decontamination

6. Spaulding Classification that is defined as coming into contact with non-intact skin

7. Type of sterilizer that aerates

9. Acronym for Safety Data Sheet

11. Pressure of Preparation Area

13. Wrapping technique frequently used for larger trays

14. Acronym for Personal Protective Equipment