


Name: _____

Date: _____

chapter 17 and 20

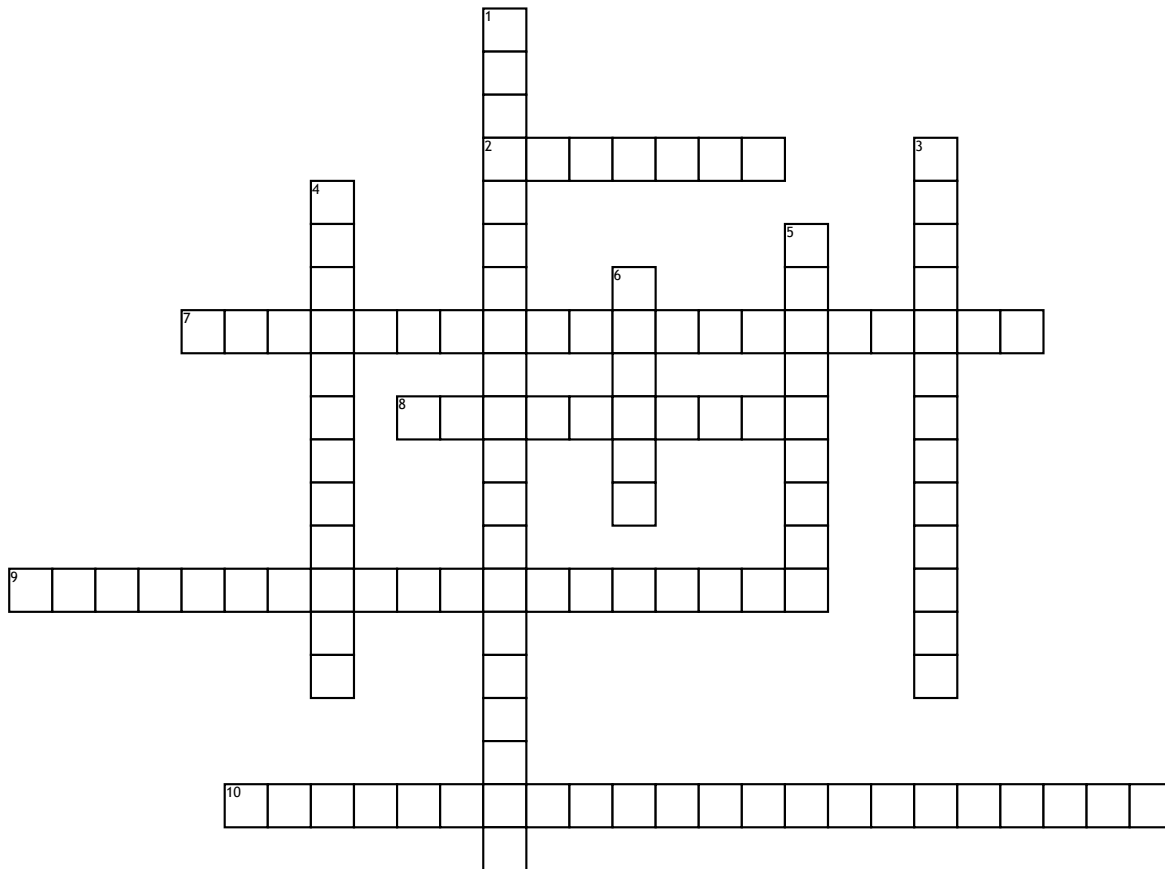

Across

2. To watch, observe, to listen to or to check (something) for a special purpose over a period of time
7. portable (mobile) equipment used in the care and treatment of patients
8. Procedures used by equipment manufacturers to obtain, record and interpret test results required to establish that a process consistently produces a sterile product
9. service provided to equipment to maintain its proper operating condition by providing planned inspection, and by detecting and correcting failures before they occur
10. label information on sterilization packages, trays or containers that identifies the sterilizer, cycle run and date of sterilization

Down

1. The hospital department responsible for performing safety inspections and function test on medical equipment
3. an area within the healthcare facility that conducts invasive and minimally invasive procedures requiring instruments, supplies and equipment
4. Procedures used by a healthcare facilities to confirm that the validation undertaken by equipment manufacturer is applicable to the specific setting
5. The number of days that that have elapsed since january 1
6. procedures used to return equipment to proper operating condition after it has become inoperative